

The worlds leading point of care test cup.

# *iCup*<sup>®</sup> & *iCup*<sup>®</sup> A.D.

Urine Drug Screening Device.




Substance abuse testing with more **substance**.

# How it works.

PRODUCT TRAINING AND  
CERTIFICATION AVAILABLE ONLINE.

## Features & Benefits

- » Integrated test cup screens for 3-13 prescription and illicit drugs
- » FDA 510(k) Cleared; CLIA Waived options available
- » Integrated specimen validity combinations available: CR, GL, NI, OX, PH, SG\*
- » Self contained cup minimizes collector exposure to urine
- » Fast results in 5 minutes

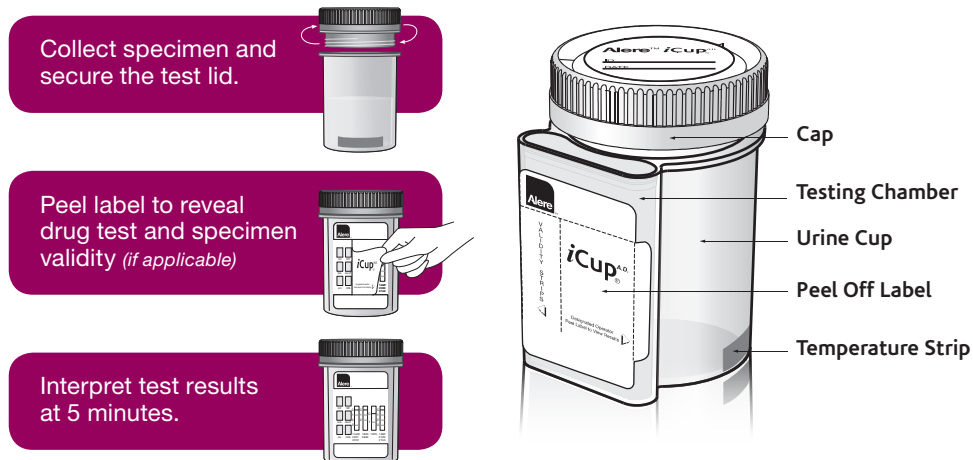

PRODUCT PROCEDURE NOTE: Refer to product insert for complete instructions, limitations, and warnings.

For in vitro diagnostic use only. This assay provides only a preliminary analytical test result. A more specific alternate chemical method must be used in order to obtain a confirmed analytical result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method. Clinical consideration and professional judgement should be applied to any drug of abuse test result, particularly when preliminary positive results are indicated.

## Urine Screening Device Cutoff Levels

Test	Calibrator	Cutoff
Amphetamine (AMP)	d-Amphetamine	1,000 ng/mL
Barbiturates (BAR)	Secobarbital	300 ng/mL
Benzodiazepines (BZO)	Oxazepam	300 ng/mL
Buprenorphine (BUP)	Buprenorphine	10 ng/mL
Cocaine (COC)	Benzoylcegonine	300 ng/mL
Cocaine (COC 150)	Benzoylcegonine	150 ng/mL
EDDP (Methadone Metabolite)	2-Ethylidene-1, 5-dimethyl-3, 3-diphenylpyrrolidine	300 ng/mL
Marijuana (THC)	11-nor- $\Delta^9$ -THC-9-COOH	50 ng/mL
Methadone (MTD)	Methadone	300 ng/mL
Methamphetamine (mAMP)	d-Methamphetamine	1,000 ng/mL
Methamphetamine (mAMP 500)	d-Methamphetamine	500 ng/mL
Methylenedioxymethamphetamine (MDMA) Ecstasy	d,l-Methylenedioxymethamphetamine	500 ng/mL
Opiate (MOP)	Morphine	300 ng/mL
Opiate (OPI)	Morphine	2,000 ng/mL
Oxycodone (OXY)	Oxycodone	100 ng/mL
Phencyclidine (PCP)	Phencyclidine	25 ng/mL
Propoxyphene (PPX)	Propoxyphene	300 ng/mL
Tricyclic Antidepressants (TCA)	Nortriptyline	1,000 ng/mL

\*Specimen validity tests: Creatinine (CR), Glutaraldehyde (GL), Nitrate (NI), Oxidants (OX), ph (PH), Specific Gravity (SG)

